


1/13

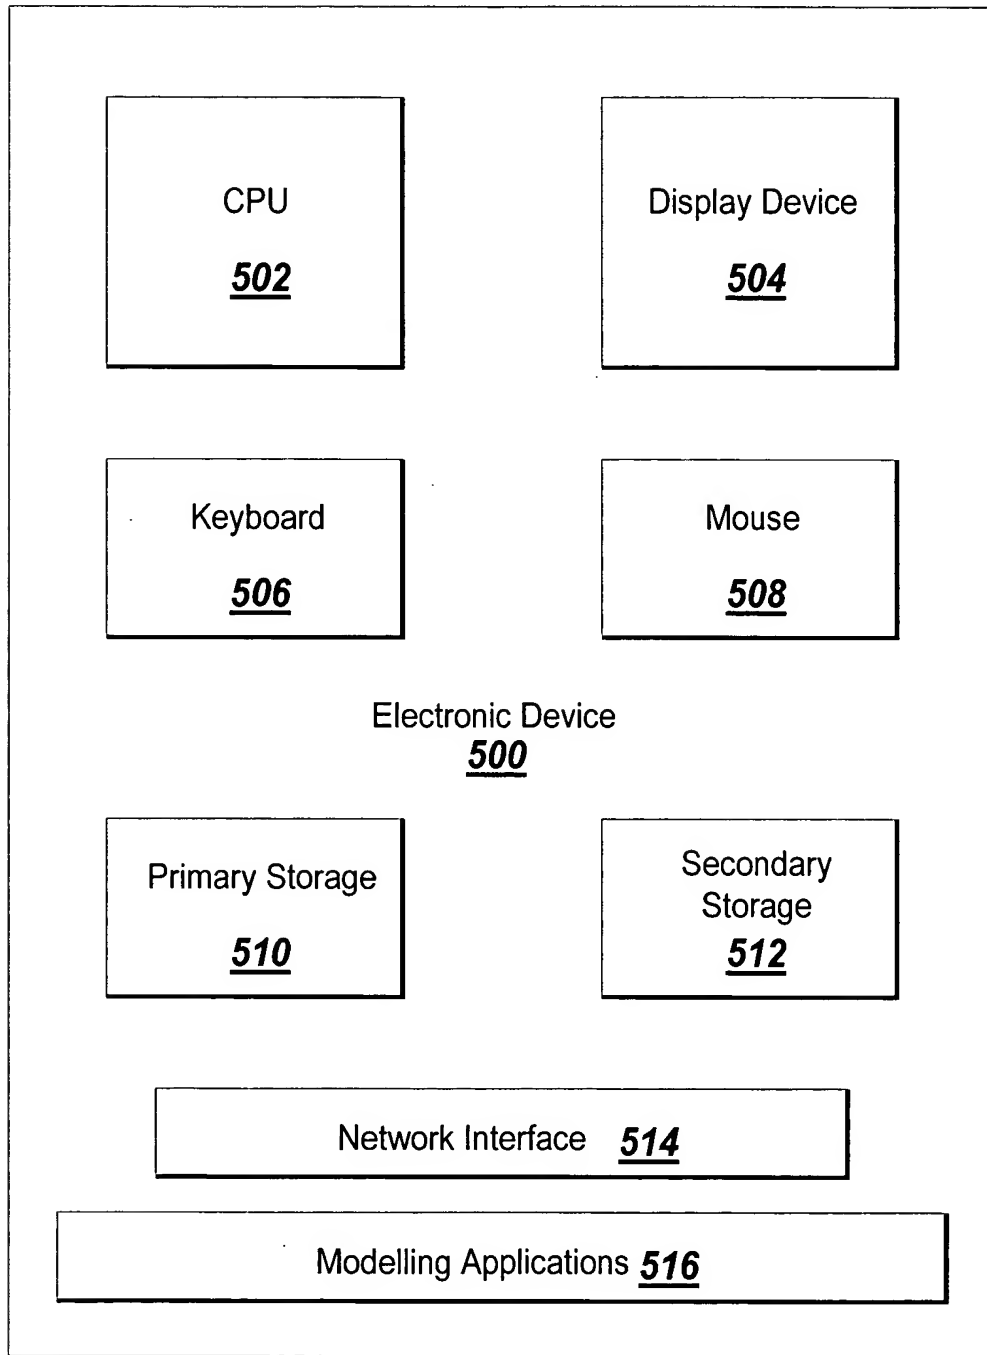

*Fig. 1*

2/13

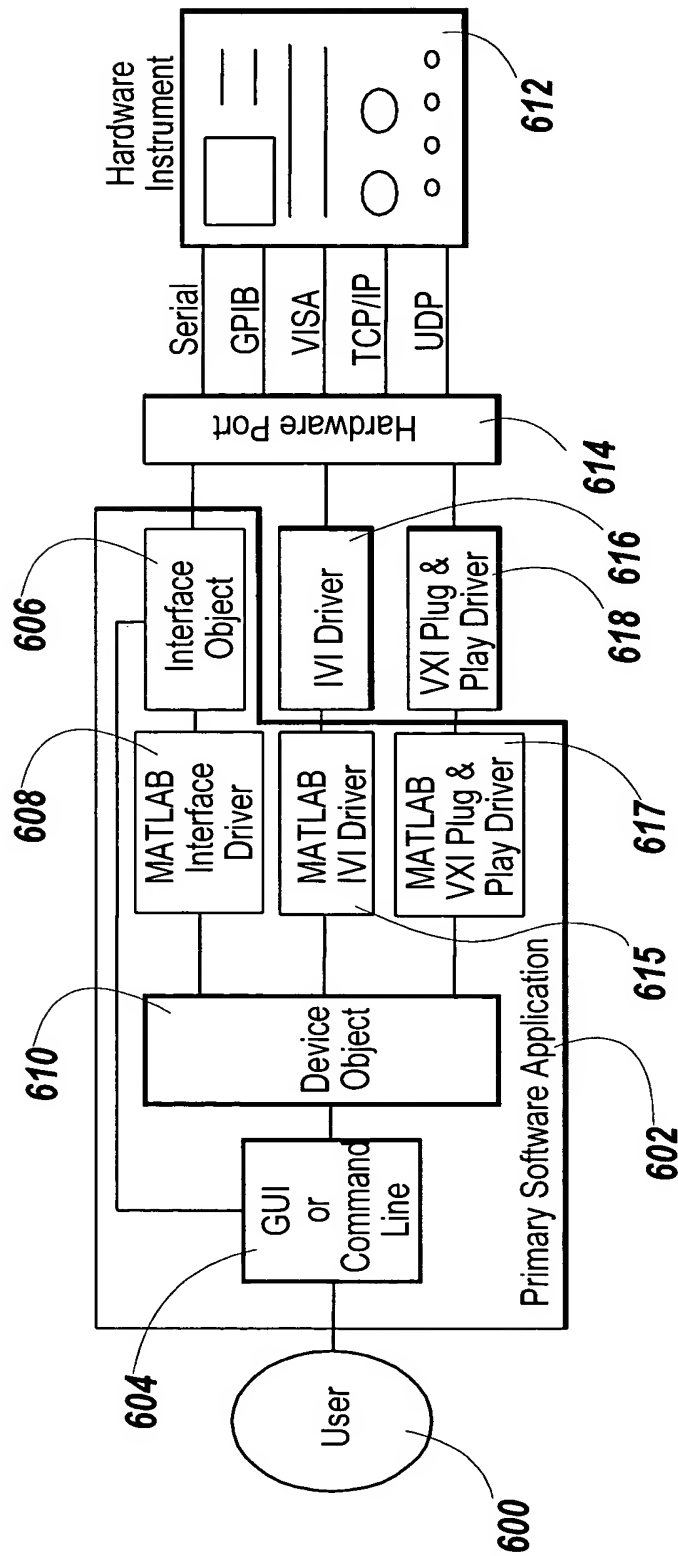


Fig. 2

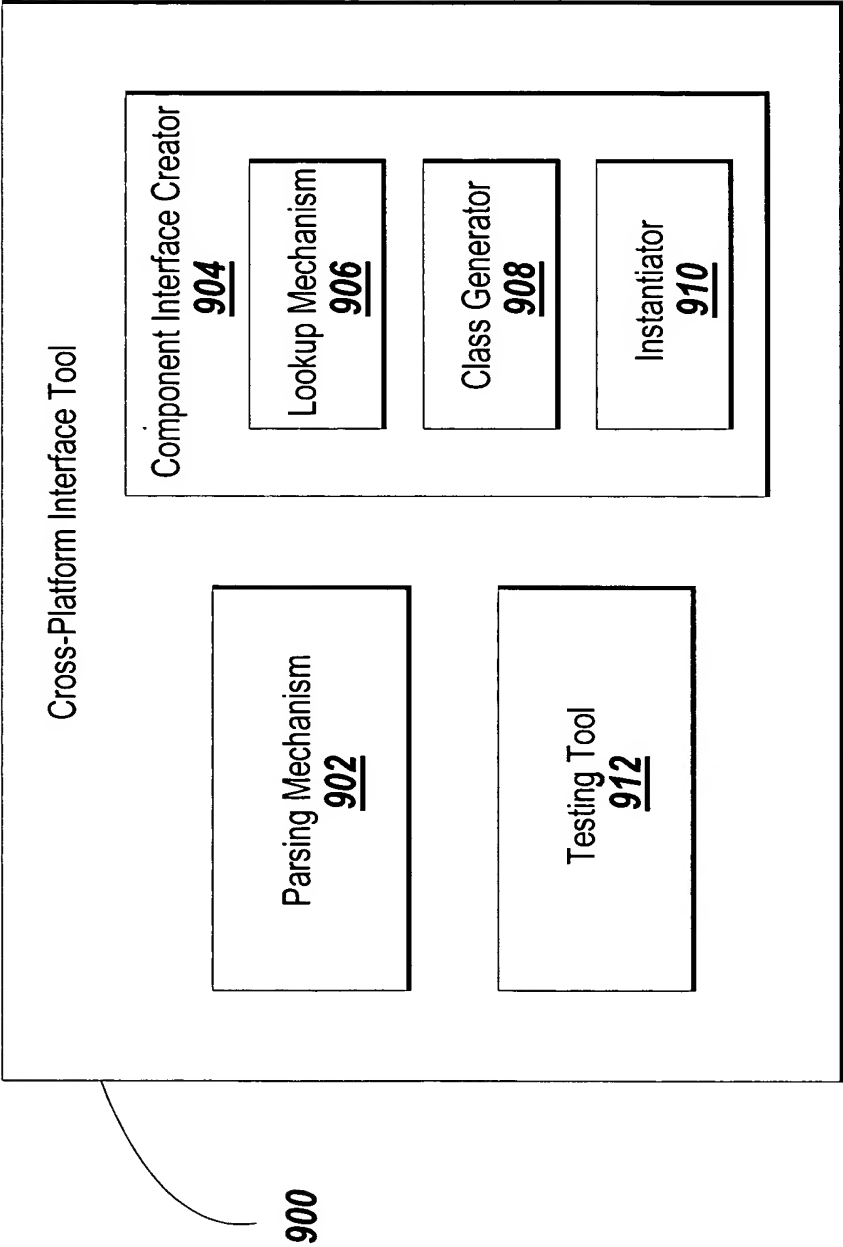


Fig. 3

4/13

630

**Block Parameters: Device Object Execute Function**

Description

Execute a device object function.

632

Parameters

Block sample time: 1

634

Device Object Instrument Initialization

Name: Unnamed test

636

Driver: D:\tek.mdd Browse...

638

Function:

Device object functions:

- calibrate
- configureWaveform
- devicereset

Function definition: [OUT1] = INVOKE(OBJ, 'calibrate')


Object: Device object

640

OK Cancel Help Apply


Fig. 4

5/13

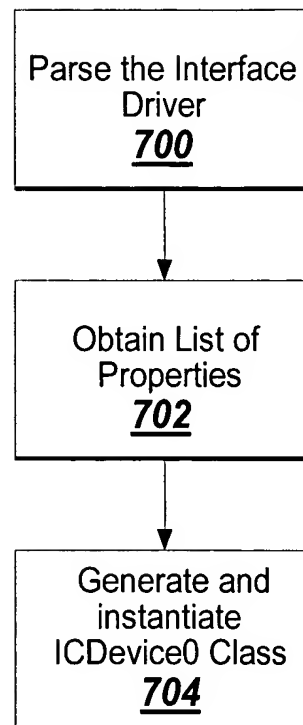


*Fig. 5*

6/13

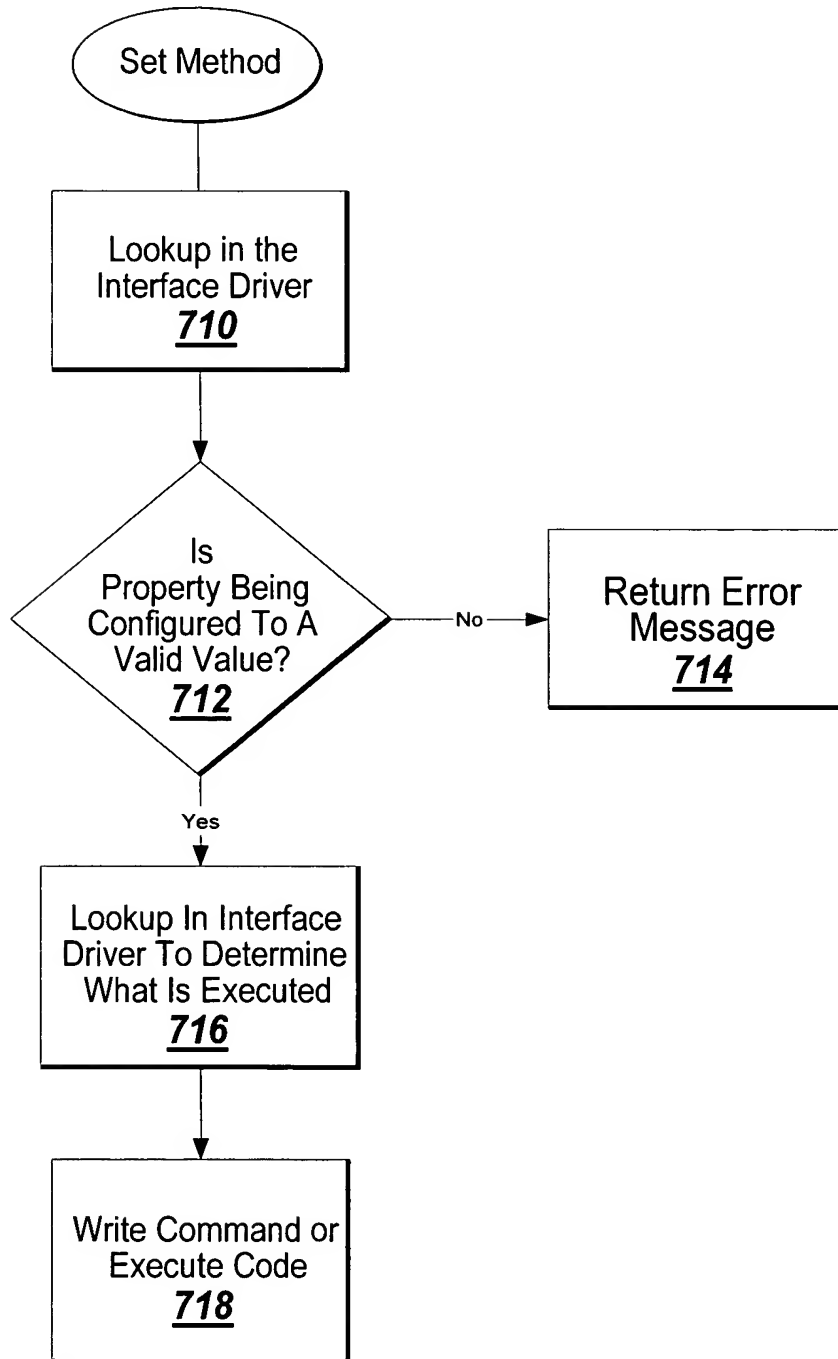


*Fig. 6*

7/13

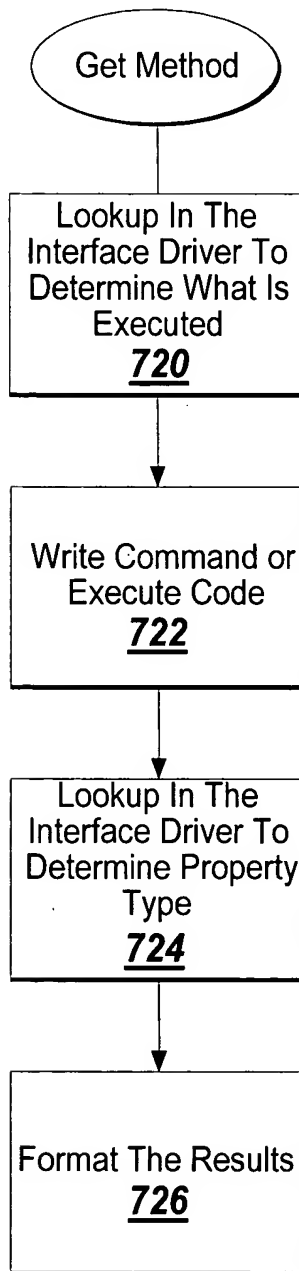

*Fig. 7*


8/13

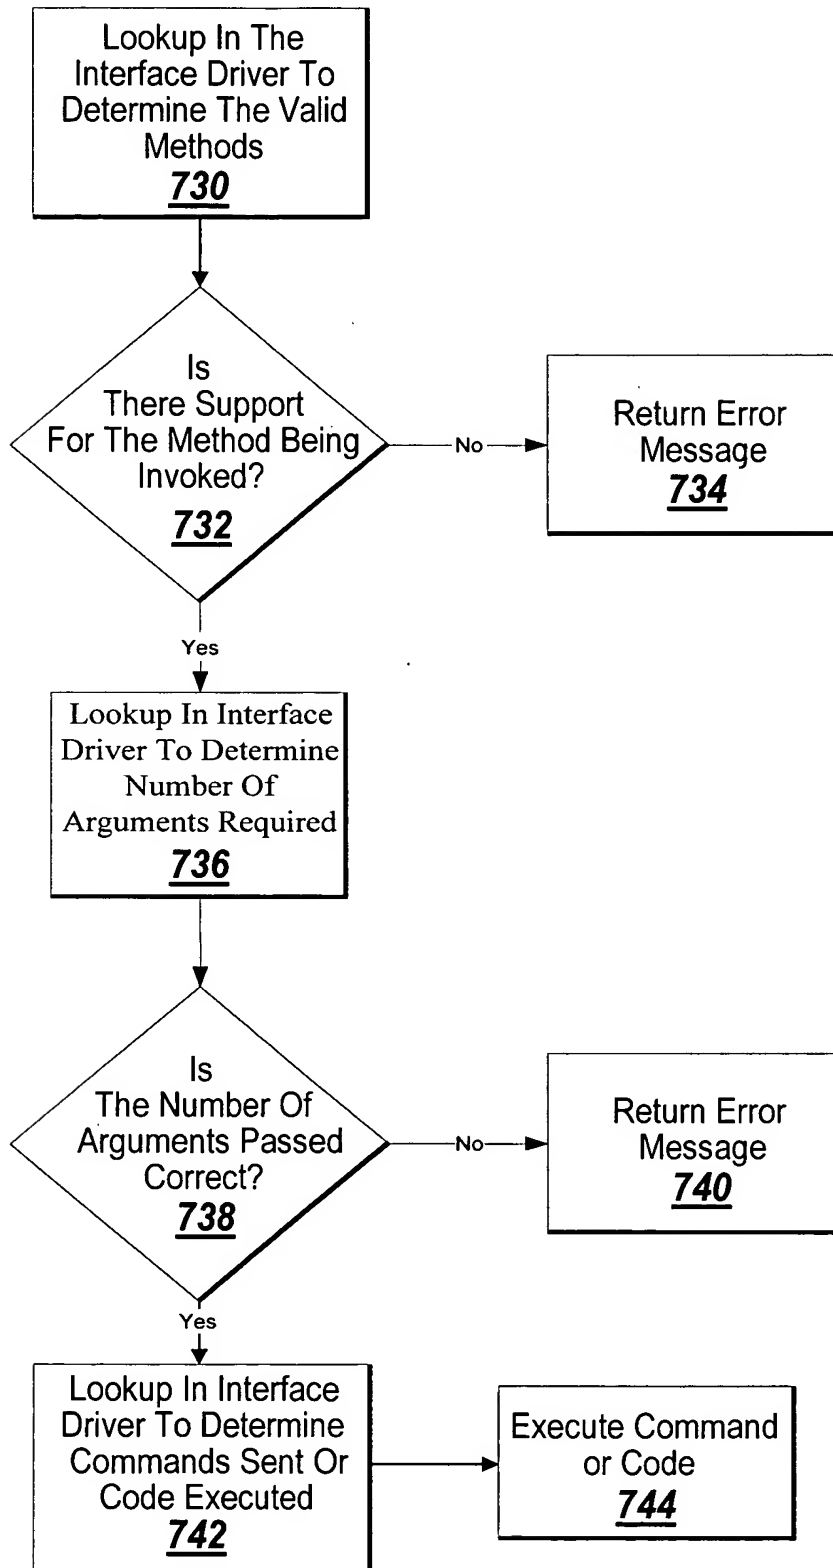

*Fig. 8*




9/13

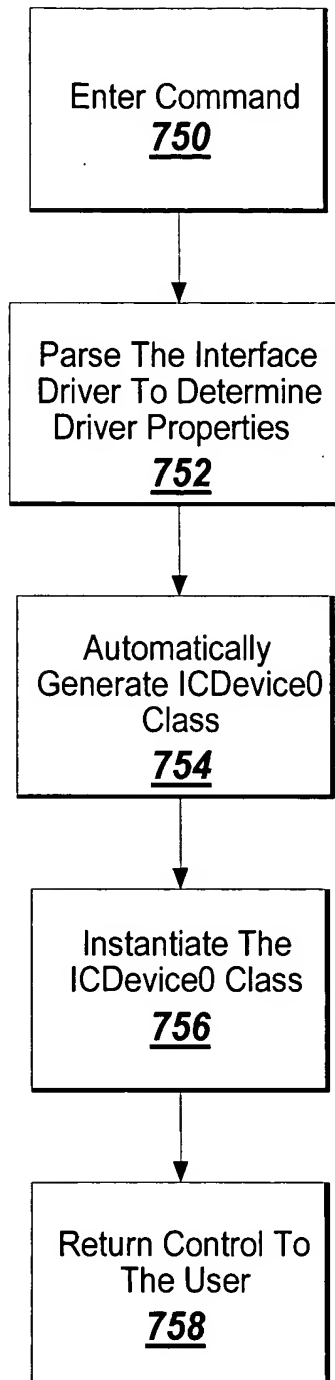


*Fig. 9*

10/13

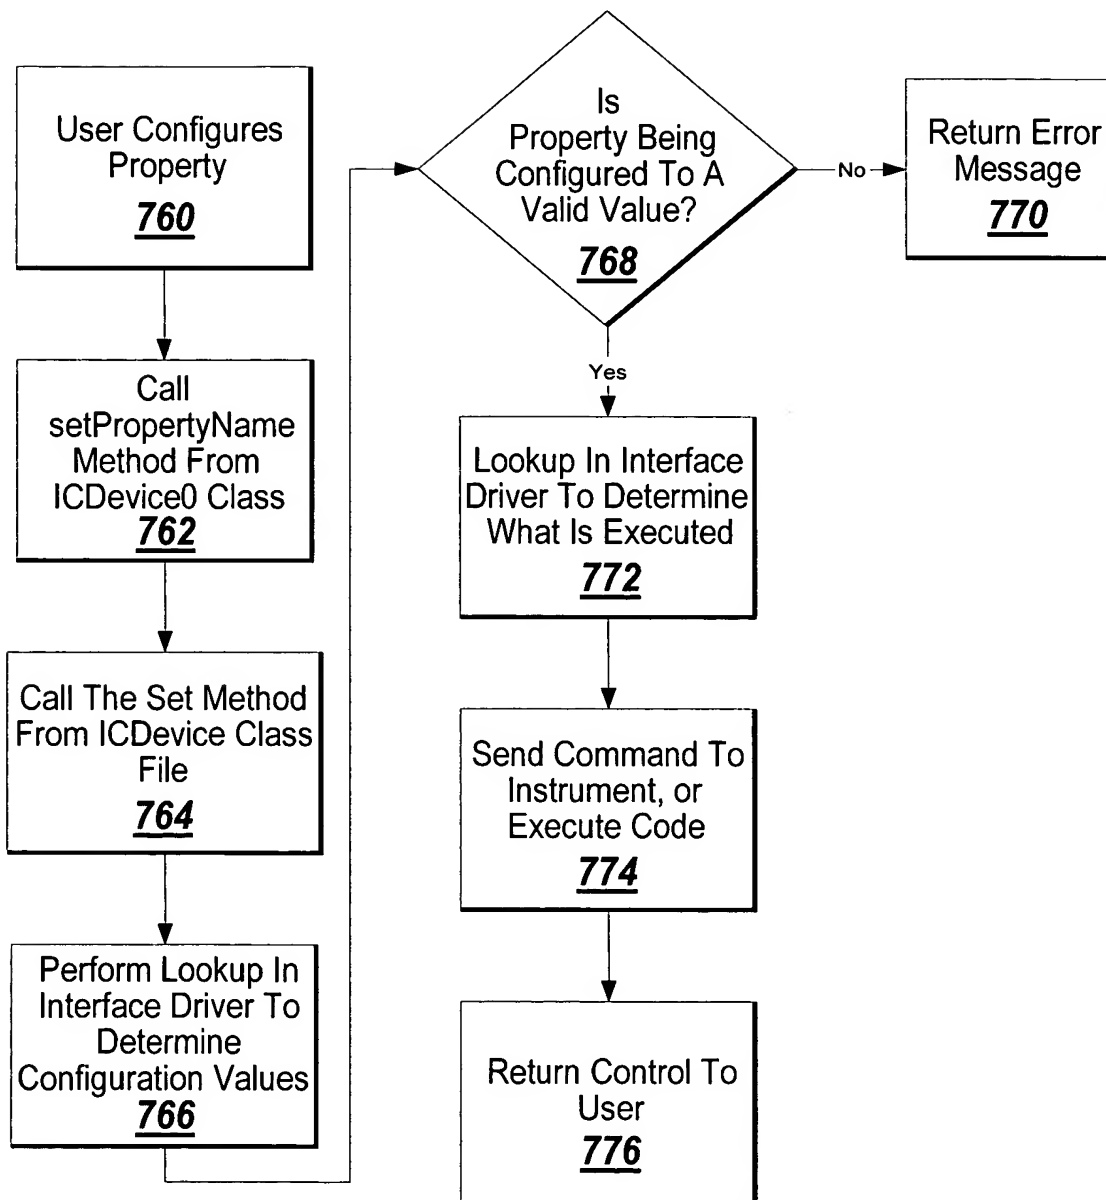


*Fig. 10*

11/13

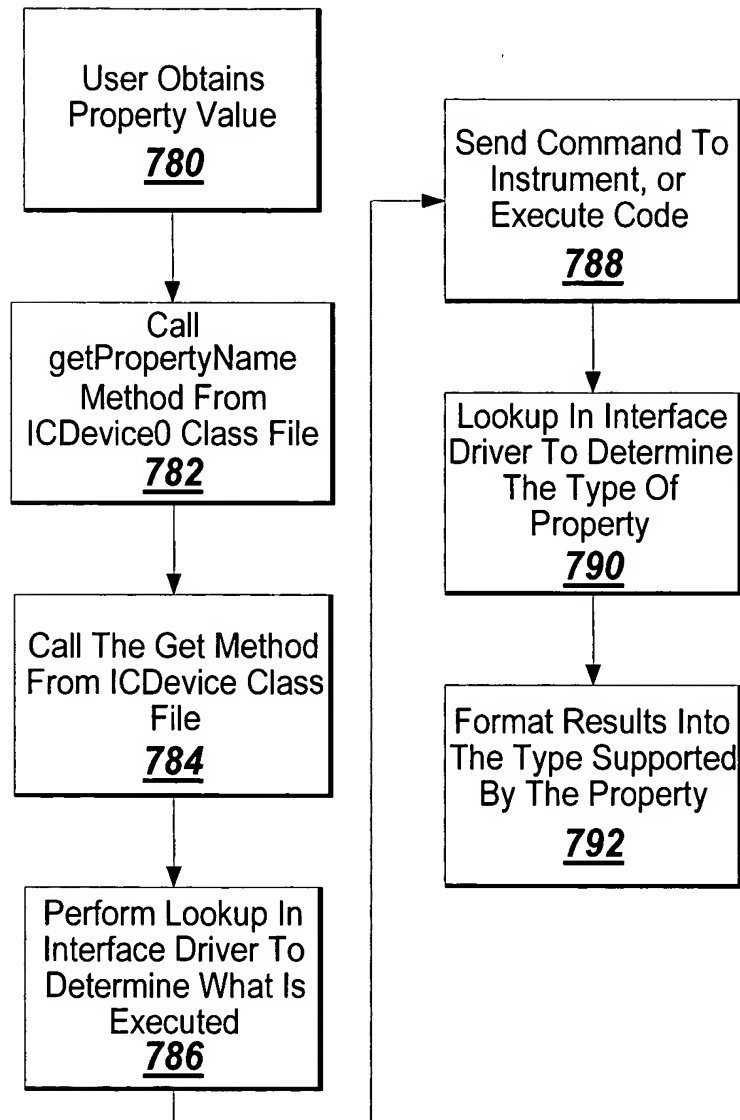

*Fig. 11*

12/13

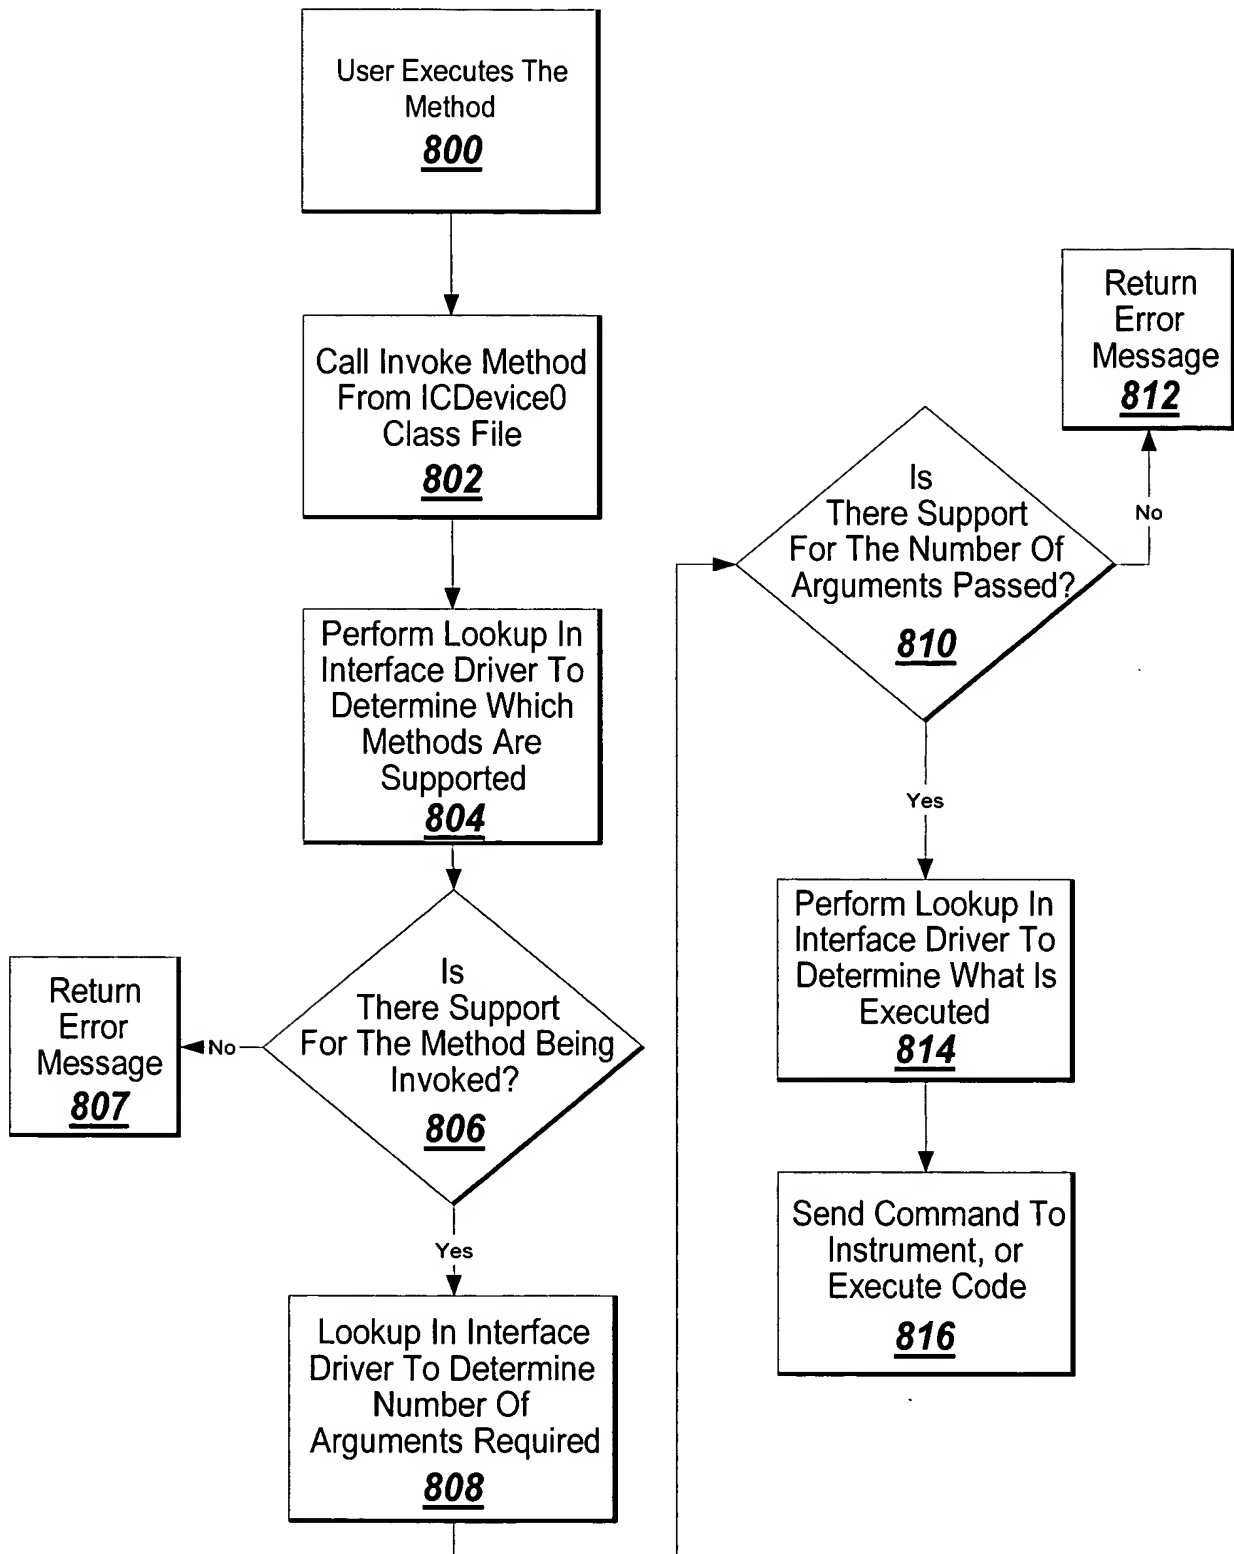

*Fig. 12*

13/13

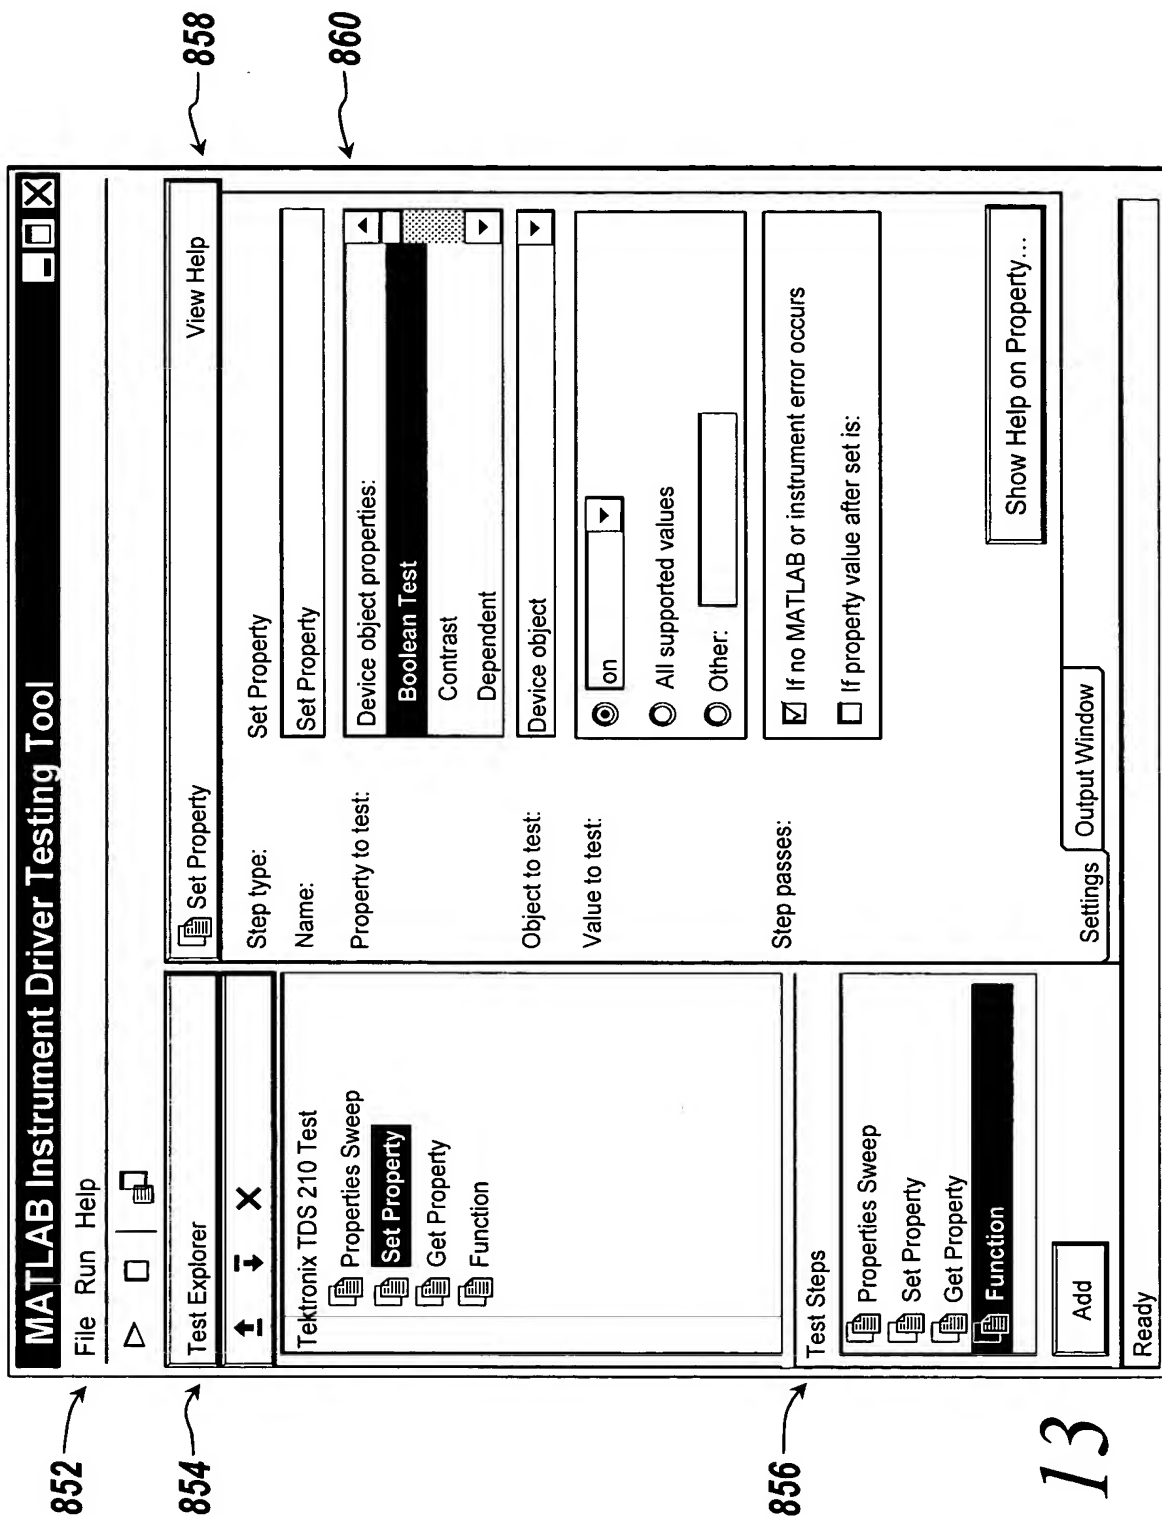


Fig. 13